

Crypto-Strip

Rapid diagnostic test for *in vitro* detection of *Cryptosporidium* in stool specimens


- Easy to use
- Easy to read
- Specific
- Sensitive
- Reliable
- Rapid (15')



www.corisbio.com



Crypto-Strip

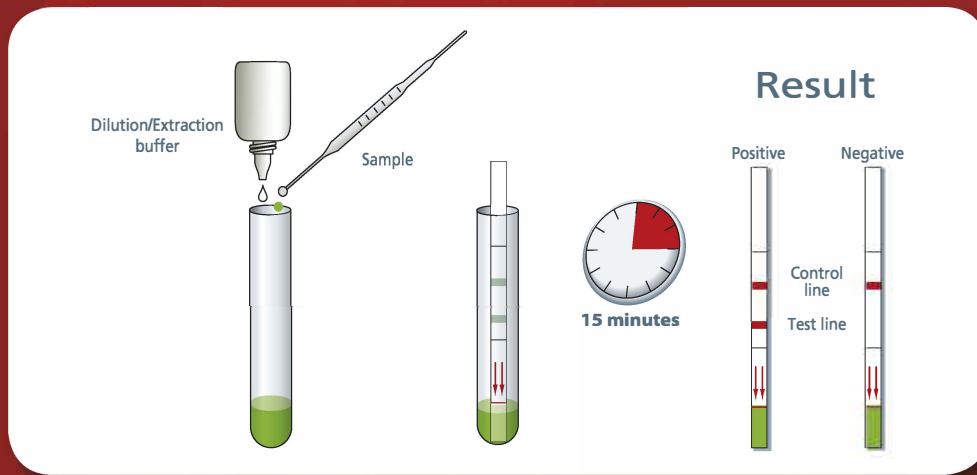

Performance compared to

	EIA (n=103)	EIA (n=100)
Specificity	100% (85/85)	100% (53/53)
Sensitivity	94.4% (17/18)	95.7% (45/47)
PPV	100% (17/17)	100% (45/45)
NPV	98.8% (85/86)	96.4% (53/55)
Accuracy	99% (102/103)	98% (98/100)

For more technical information

client.care@corisbio.com

Ordering Information

Product Name	Description	Storage	Code
Crypto-Strip	25 tests, buffer	4°C to 30°C	C-1005
Crypto Uni-Strip	10 individual strips, buffer, sample taking material (test tubes, loops, tube holder)	4°C to 30°C	C-1505

All diagnostics available in Coris BioConcept catalogue :

Adenovirus, Adenovirus (Respiratory), Adenovirus 40 and 41, *Clostridium difficile*, Bovine Coronavirus, *Cryptosporidium*, *Escherichia coli* O157, *Escherichia coli* K99, Giardia, *Helicobacter pylori*, Influenza A and B viruses, *Legionella pneumophila*, Respiratory Syncytial Virus, Rotavirus, Mefloquine, Proguanil.
Leishmania spp., *Trypanosoma cruzi*, *P. aeruginosa* efflux.

Distributed by:



Science Park CREALYS
Rue Jean Sonet 4A - 5032 Gembloux - Belgium
Ph.: +32 (0) 81 719 910 - Fx.: +32 (0)81 719 919
sales@corisbio.com - www.corisbio.com



MADE IN BELGIUM

Fo 7.5-32-05/05
January 2012