



# Pylori-Strip


**Rapid diagnostic test for *in vitro* detection of *Helicobacter pylori* antigen in stool specimens**

- Easy to use
- Easy to read
- Specific
- Sensitive
- Reliable
- Rapid (10')
- Multiple coloured lines



[www.corisbio.com](http://www.corisbio.com)

# Pylori-Strip

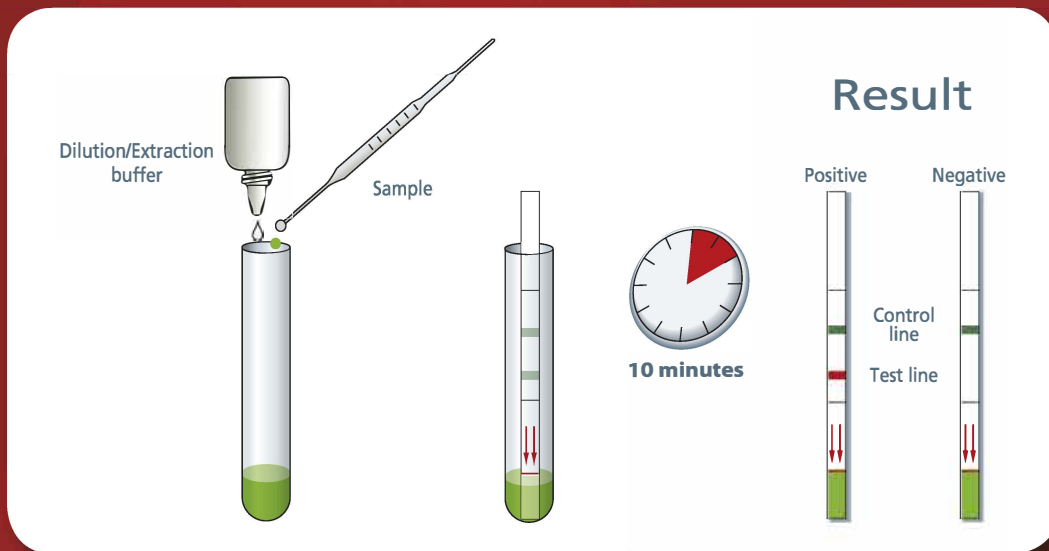

## Performance compared to EIA (n = 93)

<b>Specificity</b>	<b>97.1% (33/34)</b>
<b>Sensitivity</b>	<b>96.6% (57/59)</b>
<b>PPV</b>	<b>98.3% (57/58)</b>
<b>NPV</b>	<b>94.3% (33/35)</b>
<b>Accuracy</b>	<b>96.8% (90/93)</b>

## For more technical information

[client.care@corisbio.com](mailto:client.care@corisbio.com)

## Ordering Information

Product Name	Description	Storage	Code
Pylori-Strip	25 tests, buffer	4°C to 30°C	C-1019
Pylori K-SeT	20 cassettes, buffer	4°C to 30°C	K-1219
Pylori K-SeT	20 cassettes, 20 faecal sampling systems	4°C to 30°C	K-1519

**All diagnostics available in Coris BioConcept catalogue :**  
 Adenovirus, Adenovirus (Respiratory), Adenovirus 40 and 41, *Clostridium difficile*, Bovine Coronavirus, *Cryptosporidium*, *Escherichia coli* O157, *Escherichia coli* K99, Giardia, *Helicobacter pylori*, Influenza A and B viruses, *Legionella pneumophila*, Respiratory Syncytial Virus, Rotavirus. Mefloquine, Proguanil.  
*Leishmania spp.*, *Trypanosoma cruzi*, *P. aeruginosa* efflux.

Distributed by:



Science Park CREALYS  
 Rue Jean Sonet 4A - 5032 Gembloux - Belgium  
 Ph.: +32 (0) 81 719 910 - Fx.: +32 (0)81 719 919  
[sales@corisbio.com](mailto:sales@corisbio.com) - [www.corisbio.com](http://www.corisbio.com)

**International Medical Products S.A.**  
 Waverssesteenweg 1110/7 Chaussée de Wavre  
 OUDERGEM 1160 AUDERGHEM - BELGIUM  
 T: +32 (0)2 663 15 45 - F: +32 (0)2 660 20 98  
[www.intermed.be](http://www.intermed.be) - [info@intermed.be](mailto:info@intermed.be)

MADE IN BELGIUM

Fo 7.5-32-19/03  
 January 2012