




40/41 Adeno-Strip


Rapid diagnostic test for *in vitro* detection of group F Adenovirus in stool specimens

- Easy to use
- Easy to read
- Specific
- Sensitive
- Reliable
- Rapid (10')

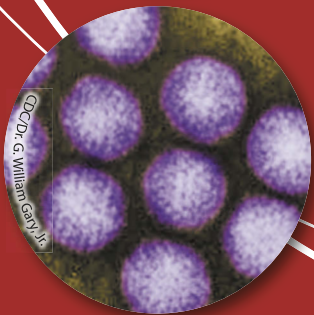

www.corisbio.com

40/41 Adeno-Strip

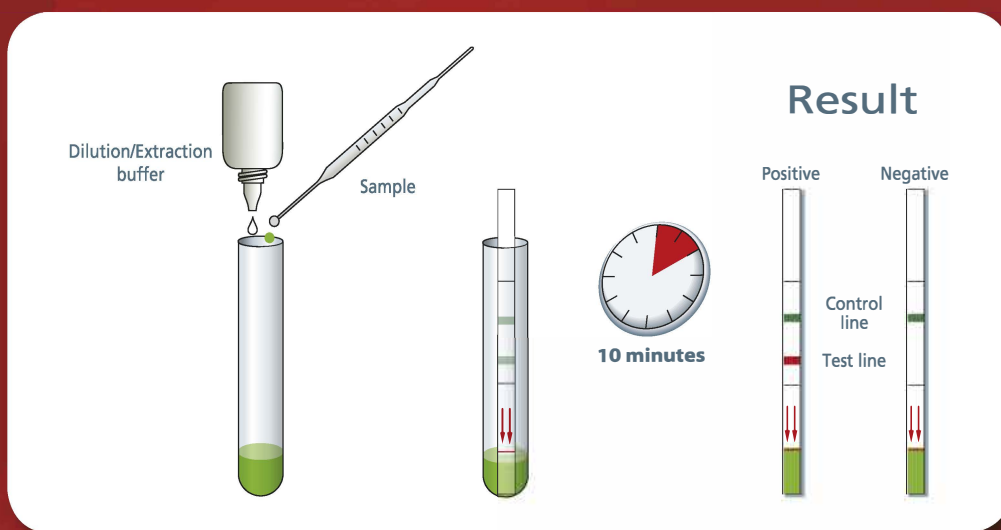

Performance compared to EIA (n = 153)

Specificity	99.3% (143/144)
Sensitivity	100% (9/9)
PPV	90% (9/10)
NPV	100% (143/143)
Accuracy	99.4% (152/153)

For more technical information

client.care@corisbio.com


Ordering Information

Product Name	Description	Storage	Code
40/41 Adeno-Strip	25 tests, buffer	4°C to 30°C	C-1003
40/41 Adeno Uni-Strip	10 individual strips, sample taking material (test tubes, loops, tube holder)	4°C to 30°C	K-1503

All diagnostics available in Coris BioConcept catalogue :

Adenovirus, Adenovirus (Respiratory), Adenovirus 40 and 41, *Clostridium difficile*, Bovine Coronavirus, *Cryptosporidium*, *Escherichia coli* O157, *Escherichia coli* K99, *Giardia*, *Helicobacter pylori*, Influenza A and B viruses, *Legionella pneumophila*, Respiratory Syncytial Virus, Rotavirus. Mefloquine, Proguanil. *Leishmania spp.*, *Trypanosoma cruzi*, *P. aeruginosa* efflux.

Distributed by:

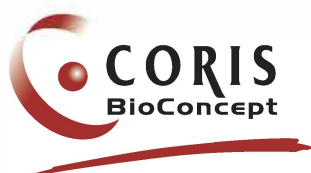

Science Park CREALYS
Rue Jean Sonet 4A - 5032 Gembloux - Belgium
Ph.: +32 (0) 81 719 910 - Fx.: +32 (0)81 719 919
sales@corisbio.com - www.corisbio.com

MADE IN BELGIUM

 **N.V. International Medical Products S.A.**
Waverssesteenweg 1110/7 Chaussée de Wavre
OUDERGEM 1160 AUDERGHEM - BELGIUM
T: +32 (0)2 663 15 45 - F: +32 (0)2 660 20 98
www.intermed.be - info@intermed.be

Fo 7.5-32-03/06
January 2012