

# Combi-Strip


**Rapid diagnostic test for *in vitro* detection of Rotavirus & Adenovirus in stool specimens**

- Easy to use
- Easy to read
- Specific
- Sensitive
- Reliable
- Rapid (10')



[www.corisbio.com](http://www.corisbio.com)

# Combi-Strip

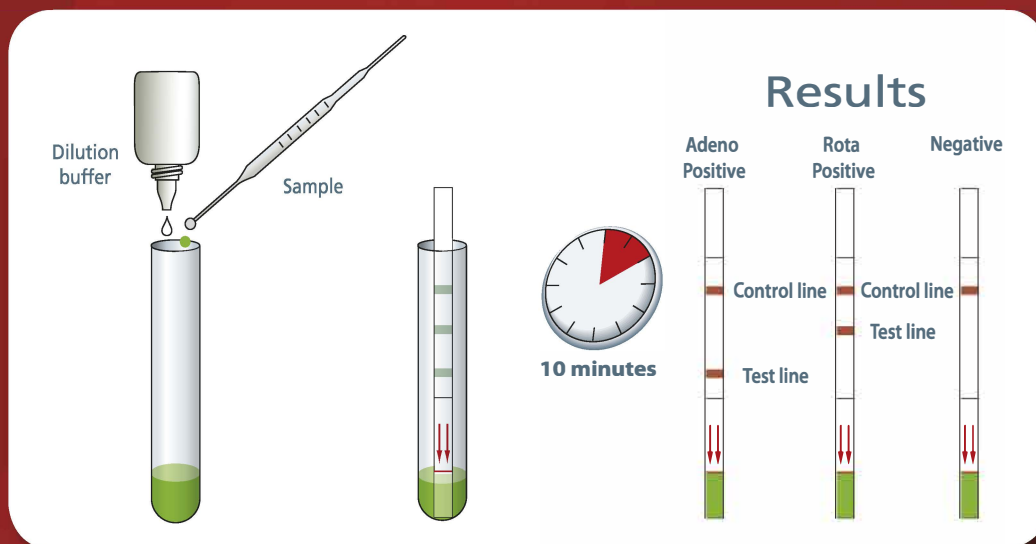

## Performance compared to EIA

	Rotavirus detection (n=214)	Adenovirus detection (n=130)
Specificity	100% (108/108)	100% (118/118)
Sensitivity	99.1% (105/106)	100% (12/12)
PPV	100% (105/105)	100% (12/12)
NPV	99.1% (108/109)	100% (118/118)
Accuracy	99.5% (213/214)	100% (130/130)

## For more technical information

[client.care@corisbio.com](mailto:client.care@corisbio.com)


## Ordering Information

Product Name	Description	Storage	Code
Combi-Strip	25 tests, buffer	4°C to 30°C	C-1004
Combi K-SeT	20 cassettes, buffer	4°C to 30°C	K-1204
Combi K-SeT, with collection set	20 cassettes, buffer, 20 faecal sampling systems	4°C to 30°C	K-1504

### All diagnostics available in Coris BioConcept catalogue :

Adenovirus, Adenovirus (Respiratory), Adenovirus 40 and 41, *Clostridium difficile*, Bovine Coronavirus, *Cryptosporidium*, *Escherichia coli* O157, *Escherichia coli* K99, Giardia, *Helicobacter pylori*, Influenza A and B viruses, *Legionella pneumophila*, Respiratory Syncytial Virus, Rotavirus. Mefloquine, Proguanil. *Leishmania spp.*, *Trypanosoma cruzi*, *P. aeruginosa* efflux.

Distributed by:

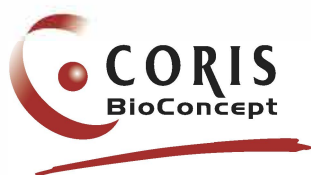

Science Park CREALYS  
Rue Jean Sonet 4A - 5032 Gembloux - Belgium  
Ph.: +32 (0) 81 719 910 - Fx.: +32 (0)81 719 919  
sales@corisbio.com - www.corisbio.com



MADE IN BELGIUM

Fo 7.5-32-04/06  
January 2012