

# Influ A+B K-Set


**Rapid diagnostic test for *in vitro* detection of Influenza A & Influenza B Viruses in swabs, washings or aspirates of nasopharyngeal secretions**

- Easy to use
- Easy to read
- Specific
- Sensitive
- Reliable
- Rapid (15')



[www.corisbio.com](http://www.corisbio.com)

# Influ A+B K-Set

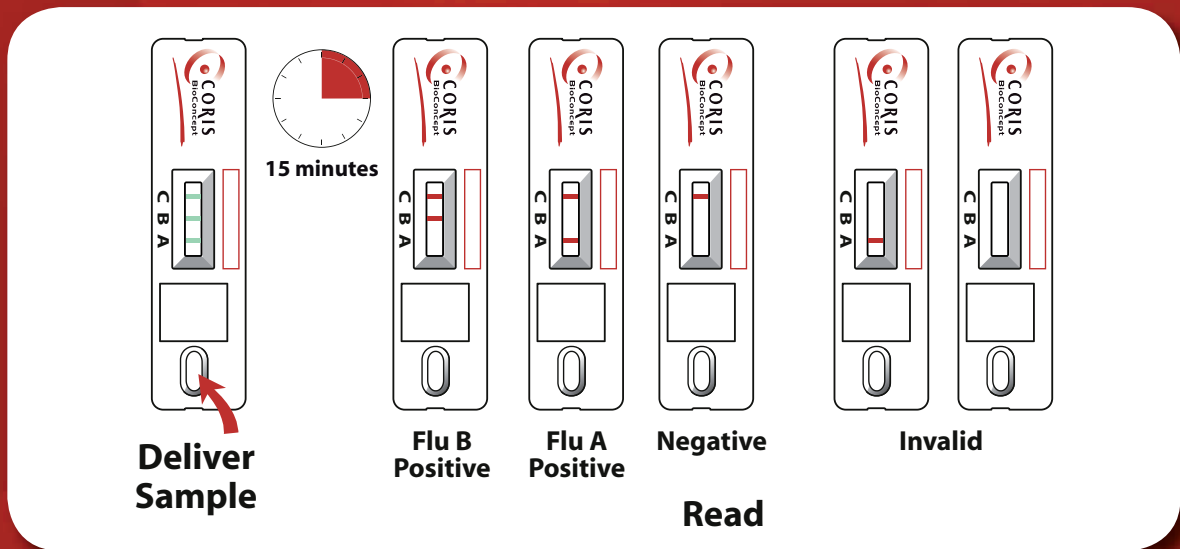

## Performance compared to Culture (n=97)

|             |       | 95% confidence interval |
|-------------|-------|-------------------------|
| Specificity | 100%  | (91.6 to 100%)          |
| Sensitivity | 90.9% | (77.4 to 97%)           |
| PPV         | 100%  | (89.1 to 100%)          |
| NPV         | 93%   | (82.2 to 97.7%)         |
| Accuracy    | 95.9% |                         |

## For more technical information

[client.care@corisbio.com](mailto:client.care@corisbio.com)


## Ordering Information

| Product Name          | Description  | Storage     | Code   |
|-----------------------|--|-------------|--------|
| Influ A+B K-Set       | 20 cassettes, buffer   | 4°C to 30°C | K-1212 |
| Influ A+B K-Set       | 20 cassettes, buffer, 20 swabs<br>20 tube-droppers   | 4°C to 30°C | K-1512 |
| Influ-A&B Respi-Strip | 25 tests, buffer   | 4°C to 30°C | C-1012 |
| Influ-A&B Uni-Strip   | 10 individual strips, buffer,<br>sample taking material<br>(test tubes, swabs, transfert pipette, tube holder) | 4°C to 30°C | C-1512 |

### All diagnostics available in Coris BioConcept catalogue :

Adenovirus, Adenovirus (Respiratory), Adenovirus 40 and 41, *Clostridium difficile*, Bovine Coronavirus, *Cryptosporidium*, *Escherichia coli* O157, *Escherichia coli* K99, Giardia, *Helicobacter pylori*, Influenza A and B viruses, *Legionella pneumophila*, Respiratory Syncytial Virus, Rotavirus. Mefloquine, Proguanil. *Leishmania spp.*, *Trypanosoma cruzi*, *P. aeruginosa* efflux.

Distributed by:

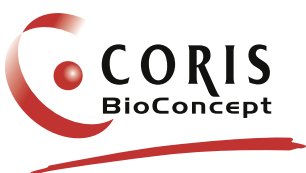

Science Park CREALYS  
Rue Jean Sonet 4A - 5032 Gembloux - Belgium  
Ph.: +32 (0) 81 719 910 - Fx.: +32 (0)81 719 919  
sales@corisbio.com - www.corisbio.com



MADE IN BELGIUM

Fo 7.5-35k/02  
October 2013