# readip

Lightweight and Portable Rapid Test Reader

#### Usage Reader for lateral flow assays Dipstick tests Test Format Results Qualitative results analysis of up to 5 test lines per dipstick 41 mm x 41 mm x 40 mm (L x W x H) Dimensions 40 g Weight LCD; 14 segment display Display User Interface One-button control Maximum 100 measurements results Memory Capacity Measuring Time Ca. 3 seconds 3 batteries CR2032 (3V/230mAh) or via Readip **Power Supply** specific data cable (optional as accessory) for connection to you PC/Laptop Interfaces 4-pol - 2,5mm jack socket for power supply (instead of batteries) and data transfer to PC/Laptop Configuration Kit-specific configuration via RFID technology Ambiant Tempera-10°C - 35°C ture (during usage) 20% - 85% Ambiant Humidity (during usage) Storage Temperature -30°C - 80°C 20% - 85% Storage Humidity

#### For More Information



+32 4 252 66 02




info@unisensor.be



www.unisensor.be



Portable Dipstick Reader

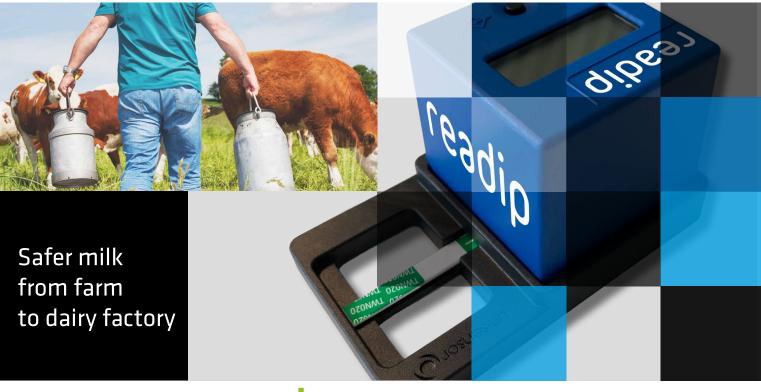











## Why readip?



SMALL

(4 x 4 x 4 cm)



LIGHT (40 g)




FAST (3 seconds)



The internal memory can store 100 results. All data can be transferred easily to a PC via a readip specific USB cable. The readip software allows a clear data presentation and remote measurements.





### What is readip?

Unisensor's readip rapid test reader offers an optimal tool for the qualitative analysis of Unisensor's dipstick tests in a small cube of only 4 cm sides.

It delivers fast and accurate results and is a cost-effective solution for any field practice. By operating with only a single button this device is especially user-friendly. Use it on a truck or in the field. Wherever you need it!

No maintenance is required. The stored data can be easily transferred to a PC via a special USB cable.

#### Now available for the following kits



#### How To Use readip



By pressing the button, you will be presented with the start screen.

Insert the test and press the

button again. Please, refer

to the Instruction For Use for

detailed information regarding

the dipstick test procedure.



The readip withhold the last reading method used. To perform a new reading, press the button again. If you want to change to another kit reference, place the RFID card on top of the readip.



The measurement is processed.



[OPTIONAL] Place the proper RFID card on the readip.



[OPTIONAL] Press the button more than 1 second if you want to check the reading method.



After approximately 3 seconds the qualitative results will scroll through the screen. The readip turns off automatically after 50 seconds.

Make sure your milk is antibiotic FREE!