





Duckworth & Kent



reusable titanium surgical instrument manufacturer

www.duckworth-and-kent.com



Instrument Care & Handling

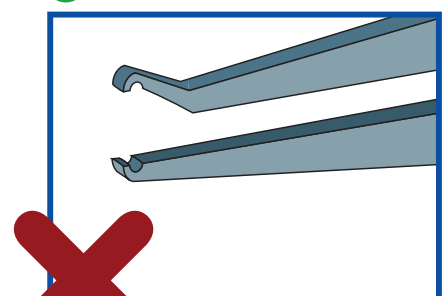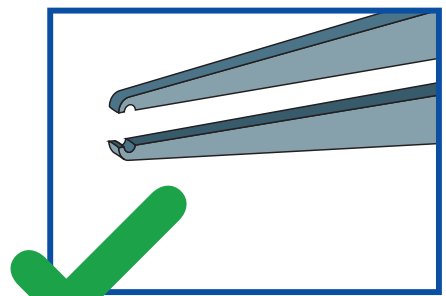



Irregular/Bent tip

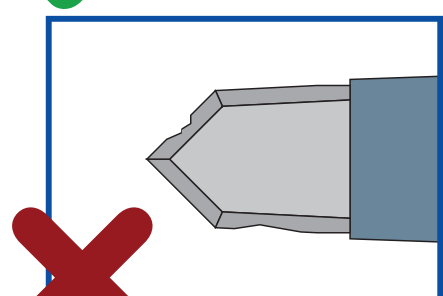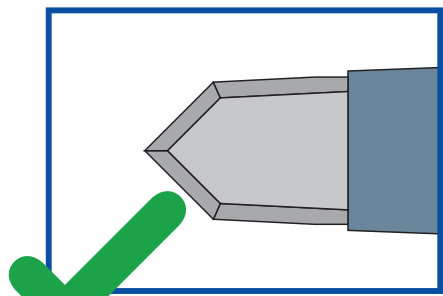



Chipped blade

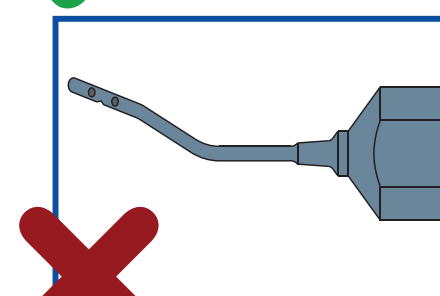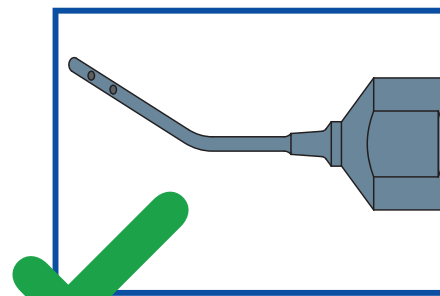



Tip bent & damaged

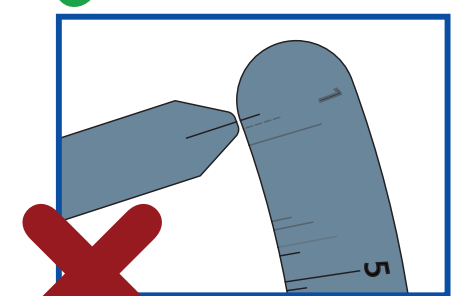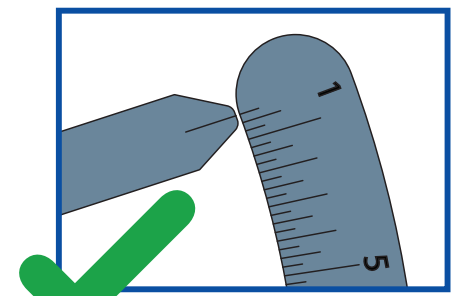



Missing graduation

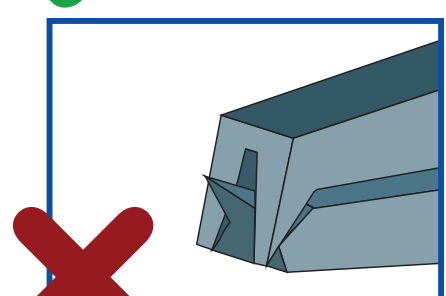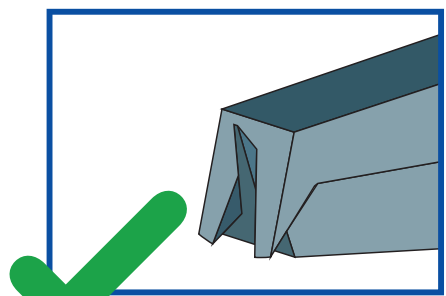



Improperly aligned tip

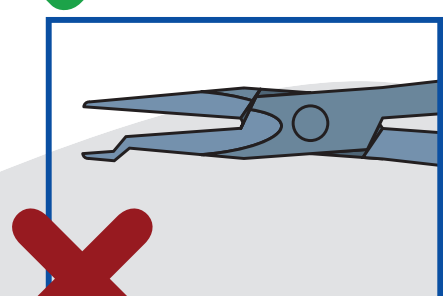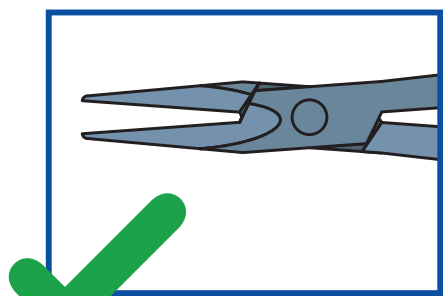



Irregular/Bent tip

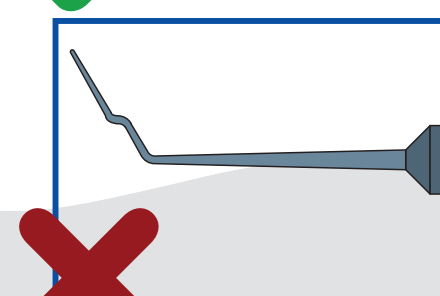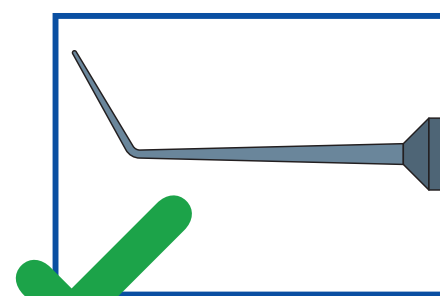



Irregular/Bent tip

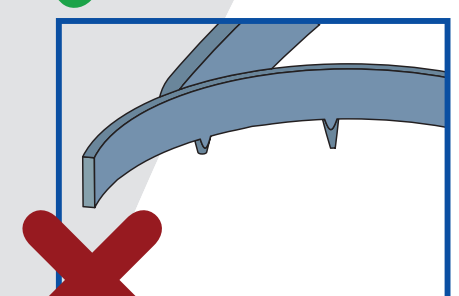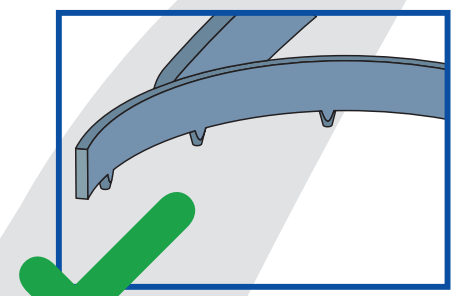



Irregular/Missing point

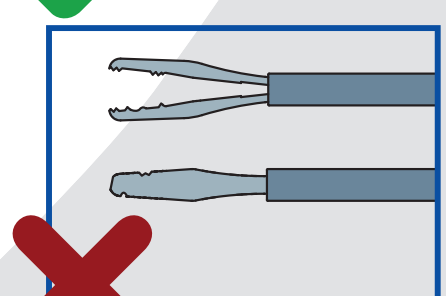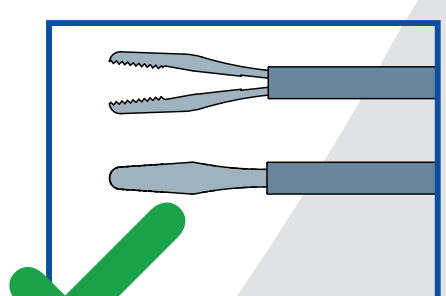



Irregular/Chipped tip

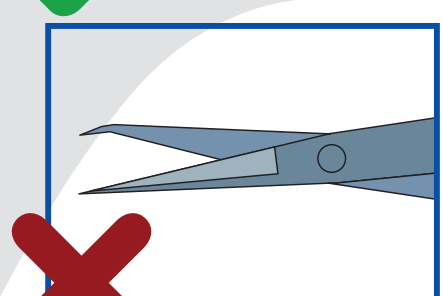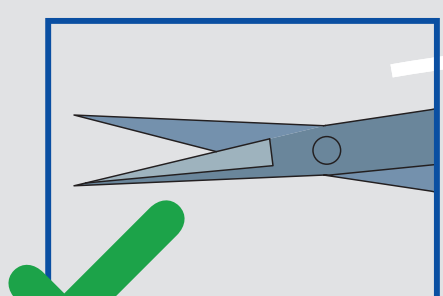

Irregular/Bent tip

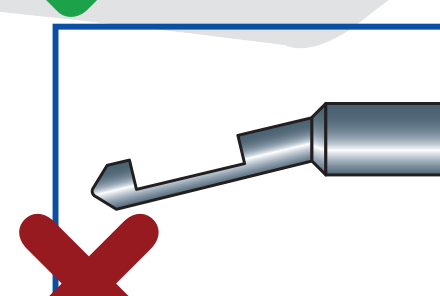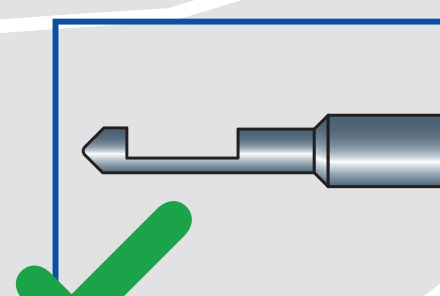

Irregular/Bent tip

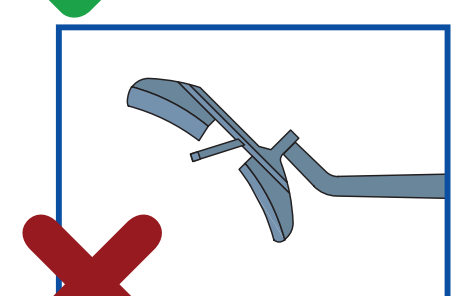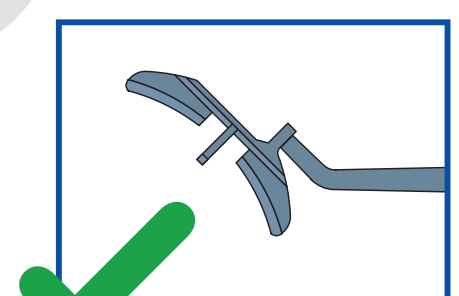

Irregular/Bent marker

Your Instrument Care is Patient Care

Distributor Details:

Lensita

Division of Luneau Technology
2 rue Roger Bonnet
27340 Pont de L'arche, France

Tel: 0032475490463
Email: alain.renson@lensita.com

